# ARC11-B PR12

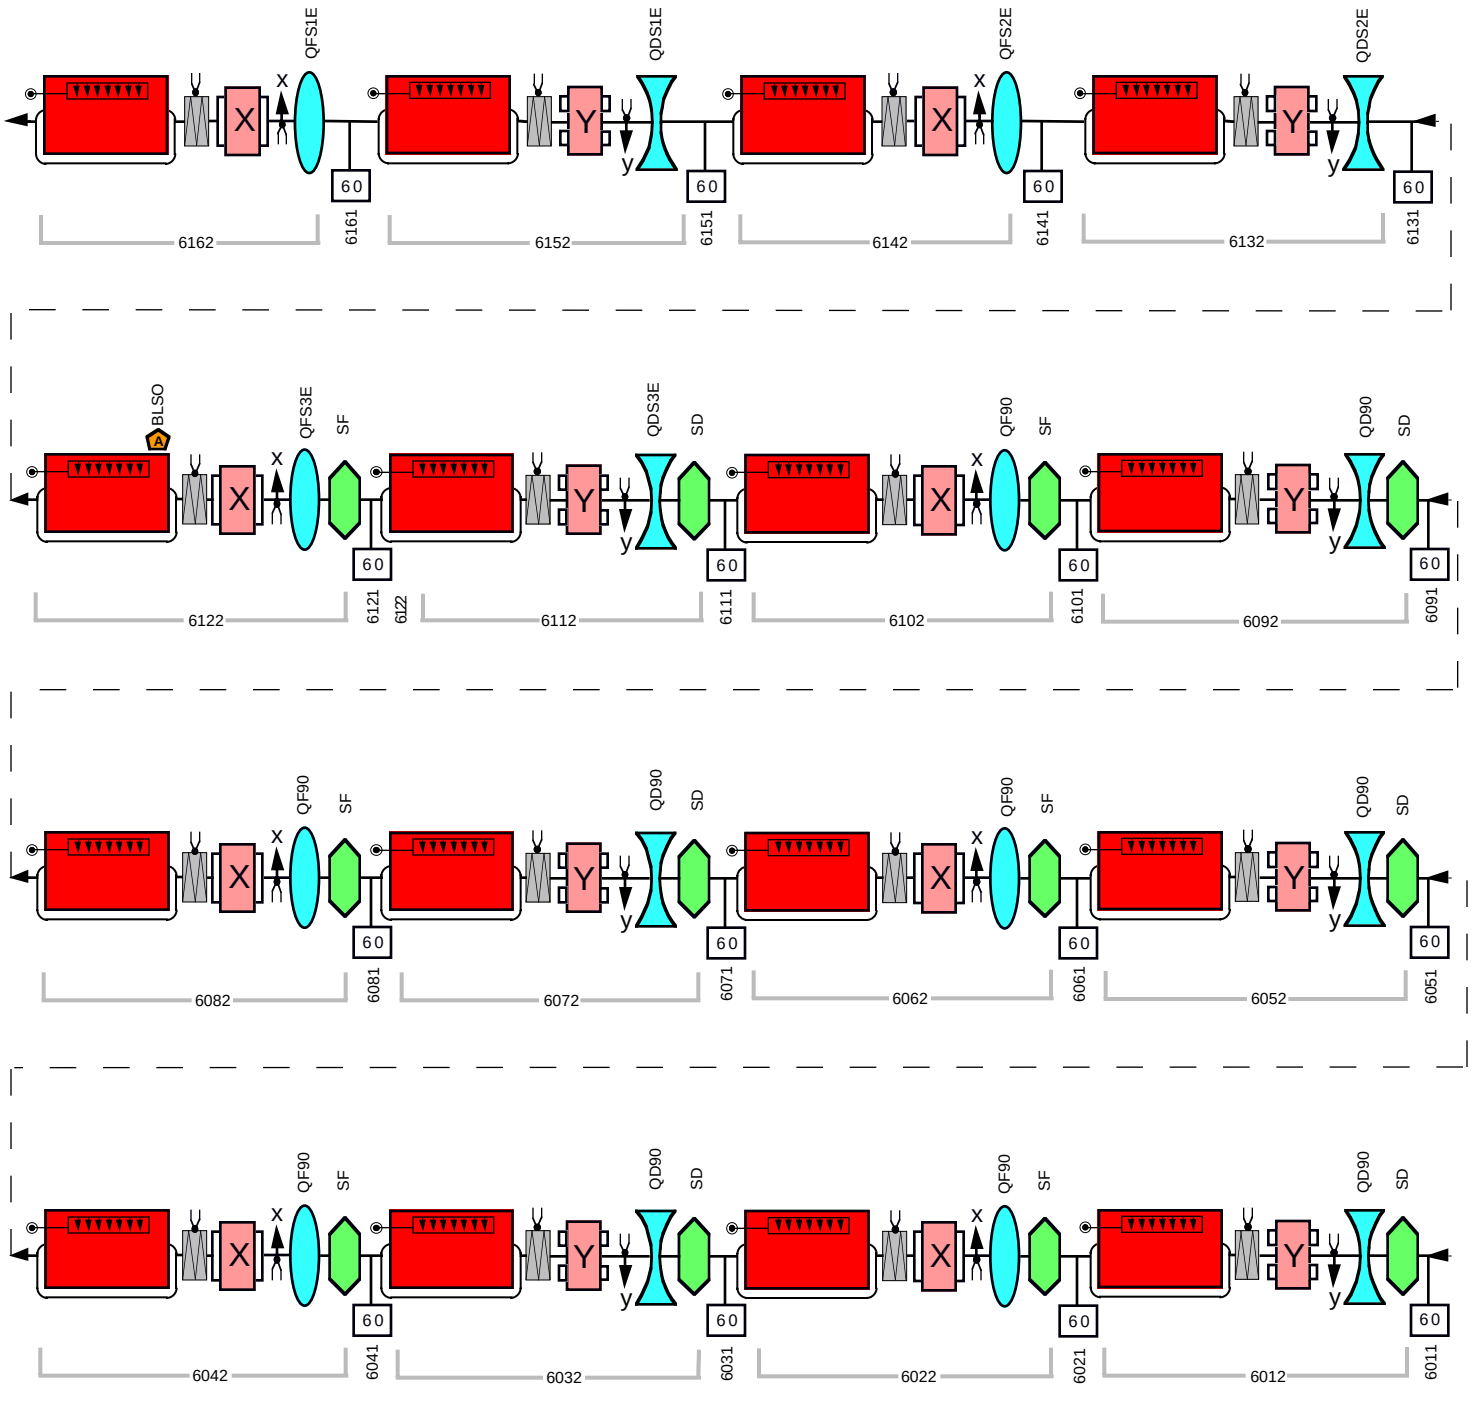


Bend magnet with DIP

Focusing quad

Defocusing quad

Horizontal corrector

Vertical corrector

Sextupole

Bellows

Horizontal BPM

Vertical BPM

Beam Loss Monitor
A-above
B-below
the beam line

Ion pump (60 l/sec)

Vacuum gauge

Thermocouple